


RifeMedic ® 7

www.rifemedic.co.za Rev 04 Jan.2021

Dual Rife Machine, Quantum Radionics Bio-Resonance Education and Application System

The RifeMedic 7 is a modern touch screen LCD multi-modality device with Educational features, Diagnosis support, Assessment and Scanner modalities, Bio-resonance applications, Health modality applications, and Tools for supporting a holistic approach to health care.

Two RifeMedic 7 LCD sizes are available: 7-inch ; 10-inch. Two RifeMedic 7 devices are offered: A double rife machine ; A double rife machine with scanner functions.

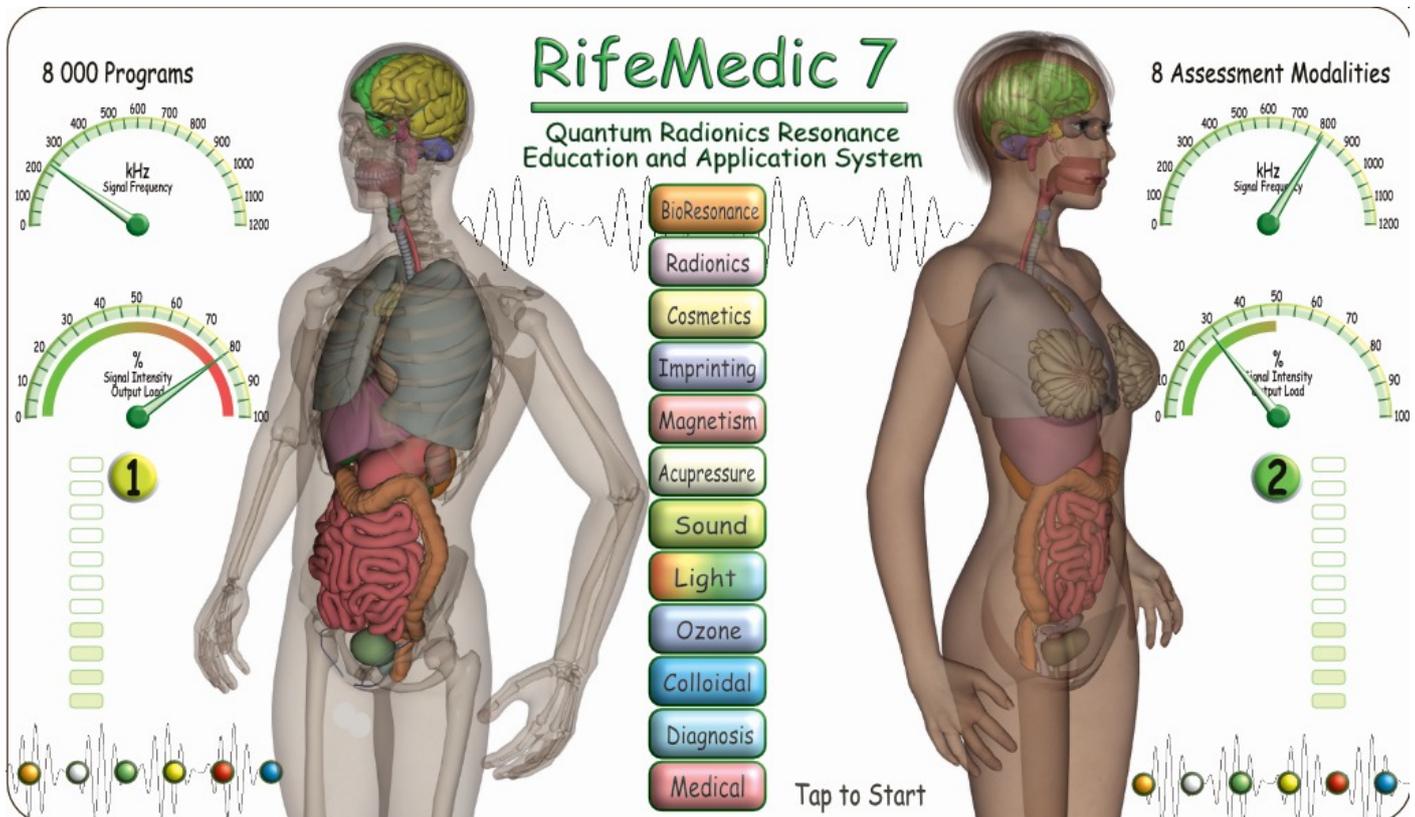

- RifeMedic 7 2XR-7 - 7" lcd dual bio-resonator
- RifeMedic 7 2XR-10 - 10" lcd dual bio-resonator
- RifeMedic 7 2XRA-7 - 7" lcd dual bio-resonator with assessment features and devices
- RifeMedic 7 2XRA-10 - 10" lcd dual bio-resonator with assessment features and devices

Features and functions of RifeMedic 7 devices are constantly being improved and updated.

Unique features include the Beat modes, Modulation modes and Position modes that have been unique features of the RifeMedic 5 devices. These modes apply dual frequency and triple frequency applications that have interestingly been recently co-discovered by other bio-resonance researchers to be extremely efficient and can not be compared with single frequency applications.

Specifications:

- 8 000 + pre-programmed rife machine programs
- 2 independent rife machine output channels
- 1 radionics and water imprint output channel (*) Note
- 8 health assessment and scanner modalities (*) Note
- 6 health support treatment modalities (*) Note
- 3 health related tools (*) Note
- 0 - 1 200 000 Hz bio-resonance frequency bandwidth per output channel
- 0 - 4 000 000 Hz bio-resonance frequency modulation system
- 48 V peak to peak maximum adjustable output per channel
- 15 nSec output switching speed

(*) Note: These features depend on the RifeMedic 7 model or may require extra devices to function.


Peripherals included: 2 x sets of hand electrodes, 1 x set of foot plates, 2 sets of connecting wires

Available peripherals: Electro-magnetic blanket, Radionics unit, Water-imprinter unit


Assessment peripherals and Tools: To be announced when ready.

Quick Start:

On all screens, press on the Man for a help screen

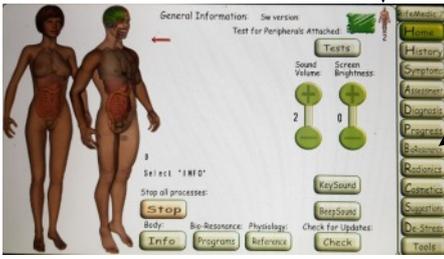

1: Press BioResonance
2: Press Programs

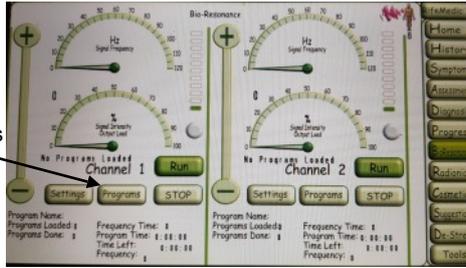


Programs Press Positions:

ON TOP is the CURRENTLY SELECTED PROGRAM

Increase the number
Decrease the number


(healing) Press the word to Search the next same word

- Go 1 Up in the list, direction = Up
- Go to Previous alpha letter, direction = Up
- Go 10 Up or Down the list
- Go to Next alpha letter, direction = Down
- Go 1 Down in the list, direction = Down

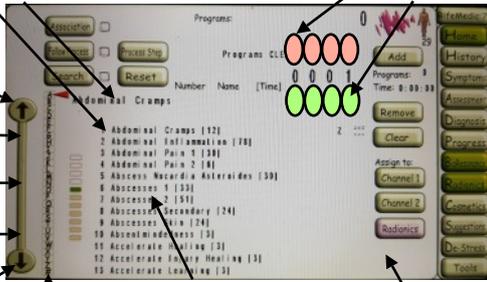

Select this Item
Select Segments of the Alphabet
Down one Page

Search

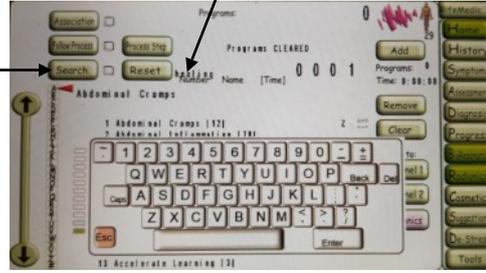


Type =healing to search for the word within the names
Select another list segment to search further from there
(go to next alpha letter and press the search word to search from there)

NB On the Programs Page: Do not make selections too fast to avoid screen sync loss - do not press wildly - take it calm

The top item is the currently selected program

3: Select and Assign Programs to one or both of the channels

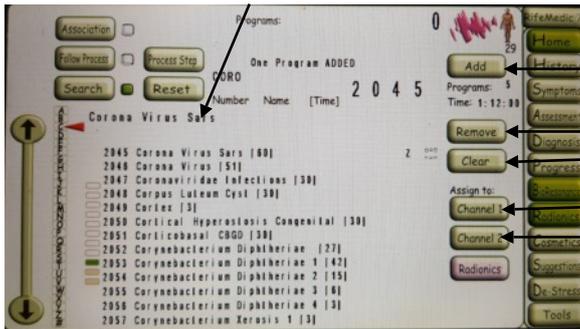

- Add the Program to the selection - the list of programs you wish to run
- Remove the last added program
- Clear the entire program selection
- Assign the selected programs to Channel 1
- Assign the selected programs to Channel 2

The procedure for assigning programs to Channel 1 and Channel 2 will be:

Add one or a selection of programs.
Assign the loaded programs to Channel 1.

Clear the selection of programs.


Add one or a selection of programs.
Assign the loaded programs to Channel 2.

Go to the BioResonance Page.

To delete programs after assigning it to a Channel, go to the Bio-Resonance Page And press the specific Channel's Stop button Twice.

Intensity select press points Automatic scale change

Remove the last added program

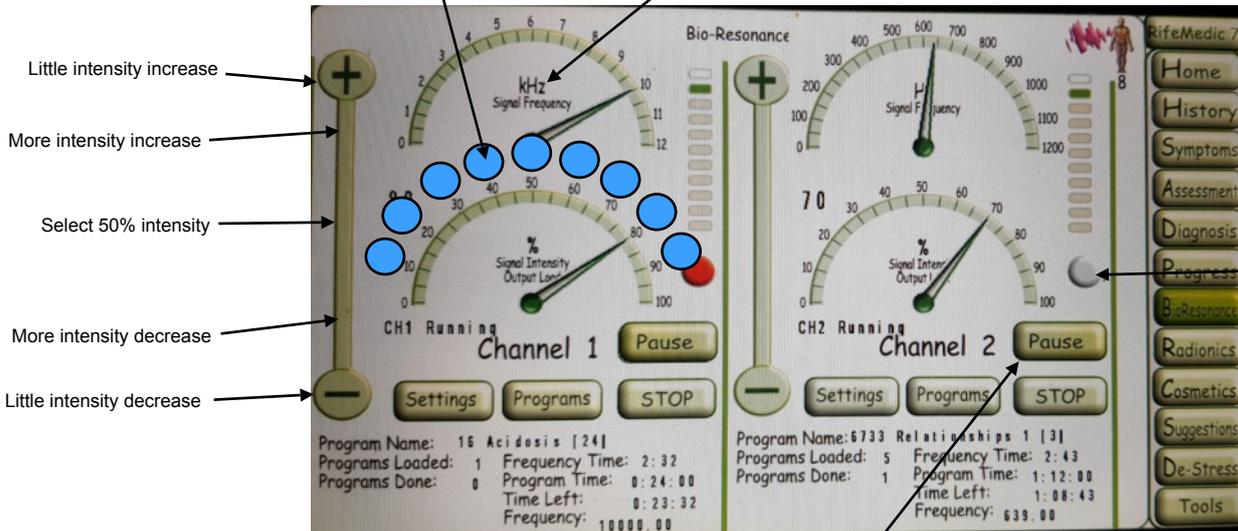

White = no programs loaded
Green = programs loaded
Pink = paused
Red = running

This button will be Run - press Run to run the Channel
Press Pause to pause the Channel - the Intensity selection will be reset

4: **While holding the electrodes in both hands or applied to both feet** - press Run and adjust the output to the desired intensity. Adjust the intensity until the sensation feels gentle and pleasant. Press intensity decrease any time while intensity increases to stop increasing or lower the intensity. Always check the output leds - they are directly connected to the electrode wires. High frequencies may not produce and sensation - do not adjust the output too high with high frequencies. Do not short out the electrodes.

5: In order to use the "Beat Mode" or the "Times Mode":

Beat Mode adds the selected frequency value of one channel to the frequency of the other channel.

For example, when you load the same programs in Channel 1 and Channel 2 like the exercise below, and you select "Beat Mode" on Channel 1 until 528 Hz appears, Channel 1's frequency = Channel 2's frequency + 528.


Times Mode multiplies the selected frequency value of one channel to the frequency of the other channel.

For example, when you load the same programs in Channel 1 and Channel 2 like the exercise below, and you select "Times Mode" on Channel 1 until 11 appears, Channel 1's frequency = Channel 2's frequency x 11.

Use only Beat Mode or Times Mode not both.

An example to let Channel 2 run 11 times faster than Channel 1:

1. Press "BioResonance" to go to the Bio-resonance page.
2. Press "Programs" to go to the Programs page
3. Press "Clear", then select your required programs for example "General Comprehensive" and press "Add" and then "Channel 1" and "Channel 2" so the same program is assigned to Channel 1 as well as to Channel 2.
4. Select the "BioResonance" page and press "Run" for Channel 1 and "Run" for Channel 2.
5. Select "Settings" and on channel 2, keep selecting "Times Mode" until the value is "11 x Frequency of Channel 1".
6. Select the "BioResonance" page and adjust the intensity of channel 1 to the point where it feels comfortable. Then adjust the intensity of channel 2 to the point where it feels comfortable. Observe the frequency of channel 2 is 11 times the frequency of channel 1.

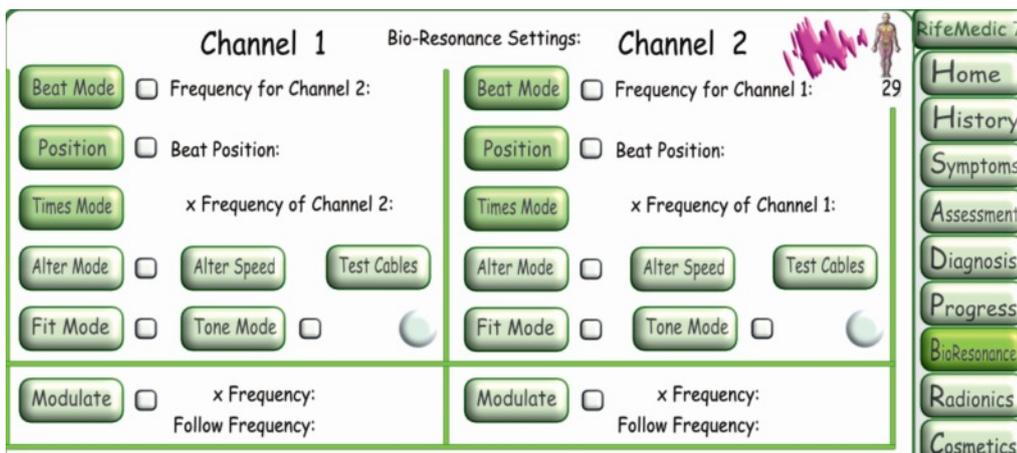

The RifeMedic 7 is a fully functional Bio-Resonance application device. It has many advanced features including a second channel that can function fully independent. Also different modes of operation and functioning for enhanced effect and other modality applications.

The RifeMedic 7 (2XR models) are development in-progress devices with new features being released about every week. Not all screens on these devices are active or usable as they may be for future implementation or only related to the more advanced scanner-RifeMedic 7 (2XRA models).

New in-progress features:

Alter Mode: Beat Mode and Times Mode Channel's frequencies are Altered or swapped

Modulation Modes: A modulation frequency can ride onto each Channel's output signal. Such a modulation frequency may enhance the currently applied frequency with an important high-frequency signal to further enhance the effect of the applied frequency.

Diagnosis Support: List your symptoms and the system will provide possible options in conditions that may associate with the symptoms.

Physiology Support: Several human physiology pages are available with vital information. Next will follow condition's effects and symptoms on the body.

User Information:

The RifeMedic 7 is a “Quantum Radionics Resonance Education and Application System”. Its Bio-Resonance application produces frequency signals in programs intended to stimulate natural functions and to support the healing processes of the body.

Please read and follow the instructions carefully. Also attend a comprehensive RifeMedic course that we offer from time to time. Web site: www.rifemedic.co.za

Who may not use this product:

(- as a general rule. In some cases, like with epilepsy, it is used to prevent a fit).

Pregnant persons; Persons using a life support system like a heart pace maker; Persons who have had a vital organ transplant like a heart, liver, pancreas, kidney, etc; Persons with a heart failure risk including hypertension, heart attack, heart cramps, heart arrhythmia; Persons suffering from epilepsy. Persons who are unsure if they should use the device. If in doubt, consult with your physician first.

Start Procedure:

- 1: Insert one cable set's banana plugs into the white sockets of channel 1, and plug hand electrodes (or foot plates) onto the other side of the cables.
2. Connect the power supply and switch on the device.
3. Follow the entry requirements - press on the startup screen, then continue and accept the conditions.
4. Observe that the red led on the front is flashing and the blue channel leds are faded and alternating at a slow rate.
- 5: Select Bio-Resonance on the right hand buttons. The screen leds will be white.
6. Select Programs and select “6 Abscesses 1 [33]” as an example exercise.
7. Select Add, then select (assign to) Channel 1. Select Bio-Resonance on the right hand buttons.
8. The screen led of channel 1 will flash green. Select Run on channel 1 and observe the frequency meter adjusts to 2720 kilohertz.
9. Hold the hand electrodes connected to channel 1 “relaxed” and adjust the output intensity: press the + - intensity adjust bar on the centre of the bar to adjust the count to 50%. press the intensity adjust bar below the + to adjust up with a fair amount or press the + to adjust a small amount. Keep on adjusting until the signal feels comfortable. Press the - position to adjust lower or above - to adjust more. Press the centre to adjust to 50%.
10. You can also press the Pause button to zero the output and stop the program from advancing. The Pause button will change to Ready. Selecting Ready will continue the program but you have to re-adjust the intensity.
11. Press STOP twice to stop the program. (The first Stop press also places the unit into Pause mode).
12. You can switch off the unit at any time.

Important matters and problems:

On the Programs Page, to avoid screen data sync loss, do not make selections too fast. Do not press wildly. If the screen freezes up, you will have to reset the device. This problem will be fixed in due time.

Certain frequencies may be extremely high. In these few cases, the output intensity adjustment will limit to 50%.

The load scales do not show due to chip software problems. This will be fixed in due time.

Certain functions on the device will be made available in due time.

Frequently Asked Questions:

The Right top RifeMedic button selects the RifeMedic page with References and more FAQ's.

Q. The RifeMedic unit does not power up. What could be the problem?

A. Check that the mains switch to the power supply is switched on and that the mains power is on (you have electricity). Check that the supplied 24 Volt power supply plug is nicely connected to the unit. Check that the unit is switched on. Check the fuse: Make sure to unplug the mains cable from the mains power supply before you open the fuse holder. You can have the power supply tested with a volt meter.

Q. The output signal leds come on but I feel no sensation.

Q. The output signal leds come on and I feel unpleasant on and off signal sensations.

A. One or both of the signal cables may be damaged and is not making contact or the contacts on the plugs may be intermittent as a result of the damage in the plugs or signal cable. Also keep in mind that you can not feel high frequencies, therefore test the unit on low frequencies like with the 6 Abscesses program.

Q. Can I cause damage by using the wrong program?

A. When standard bio-resonance principles are followed, it is unlikely that any damage will take place as most frequencies of the different programs overlap.

Q. Can I over-apply bio-resonance?

A. Yes. Commonsense should always be used. Care should be taken with the Detoxify programs, not to detoxify too fast. Also support the body during detoxification programs, for example with liver and kidney support supplements and enough water. Organs and glands should not be over-stimulated. In case of infections, depending on how acute it is, over-stimulation may worsen a condition.

Q. How will I know when I should end the application for a condition?

A. Normally when the condition has become much better, allow your body to progress with its own healing process. Support the body with immunity system enhancing supplements and good nutrition.

Q. Should I end the medication prescribed by my physician?

A. No. We recommend that you always follow the professional instructions from your doctor. We are however in general against the over-use of pain killers, anti-histamines, antibiotics, anti-depressants, sleep medication, and any medication that has negative side effects. Use your own discretion and do research.

Q. Can I use the RifeMedic when I sleep?

A. As a general rule, not during your night's sleep as many active healing and relaxation processes are taking place in the body.

Q. How can I know more about the application of bio-resonance?

A. Attend one of our comprehensive RifeMedic bio-resonance courses that are presented during the course of the year. Check on the unit, the top RifeMedic button has references and also FAQ's.

Q. I am pregnant. Can I use bio-resonance for a condition?

A. No. Please check all the conditions mentioned in the "Who may not use this product" section.

Q. Can I treat other people with my RifeMedic device?

A. No. Unless you are a health practitioner, your RifeMedic device is for your own personal use.

Q. What approach has the best result for a healthy body or for healing?

A. As the RifeMedic bio-resonator supports the body in many ways, it lacks vitally important matters like hydration, nutrition, and herbal medicines. When utilising herbal medicines, always ensure to check the contra-indications to allopathic medication. Also have a professional health practitioner support your efforts and provide you with important requirements.

Q. What other factors should be considered and observed for obtaining the best result for a healthy body or for healing?

- A.
- Body pH - must be normal - not acidic and not alkaline.
 - Blood viscosity - blood thickness has to be normal - not thick and not too thin. Most people suffer from thick blood. Do not thin blood with non-applicable allopathic medication. Consider natural herbal applications like ginkgo biloba - study the product and use it carefully to prevent over-doing it.
 - Digestive system - everything depends on this system - eat healthy, chew food for longer, control stress.
 - Immunity - support this system by supplementing with vit C, D, zinc, etc.
 - Detoxification, parasite care.
 - Emotional matters, relationships and more - many of these matters are "your decision" based.
 - Stop unnecessary bad habits like smoking, alcohol abuse, medicine abuse.
 - Work on bad stress as it inhibits digestion and promotes many unhealthy factors.
 - Exercise a little - rope skipping is the best.
 - Be treated - massage is the best health enhancement therapy being done with black cumin oil.
 - Use natural healing foods and herbs to support body weaknesses - it works slowly but man bring about permanent healing.
 - Use your RifeMedic 7 bio-resonator and all the healing, caring and supportive functions.

Contact Details: Innovation Instruments, Tel: 011 794 2751 during business hours.

Web site: www.rifemedic.co.za

Email address: modeltec@icon.co.za or pieter@innovationinstruments.co.za